

# CENTER OF MASS MOVEMENT ESTIMATION USING AN AMBULATORY MEASUREMENT SYSTEM

Schepers HM<sup>1</sup>, van Asseldonk EHF<sup>1</sup>, Buurke JH<sup>2,3</sup>, Veltink PH<sup>1</sup>

<sup>1</sup>Institute for BioMedical Engineering (BMTI), University of Twente, Enschede, The Netherlands

<sup>2</sup>Roessingh Research and Development, Enschede, The Netherlands

<sup>3</sup>Roessingh Rehabilitation Center, Enschede, The Netherlands

## INTRODUCTION

Traditionally, human body movement analysis is done in so-called ‘gait laboratories’, where several gait variables are estimated by measurement systems such as optical position measurement systems, EMG or force plates. A major drawback of these systems is their restriction to the laboratory environment. Therefore research is required for the development of measurement systems to perform these measurements in an ambulatory environment.

An important variable to characterize human walking is the Center of Mass (CoM), an imaginary point at which the total body mass can be assumed to be concentrated. Several methods exist for CoM estimation, of which the segmental kinematics method and the double integration of ground reaction force method are the most important ones.


The objective of this study is to estimate the CoM trajectory using an ambulatory measurement system which fuses Center of Pressure (CoP) trajectory with double integrated acceleration obtained from Ground Reaction Force (GRF) data. The accuracy of the ambulatory system is verified by comparing it to an optical reference system based on the segmental kinematics method

## METHODS

The measurement system consists of an orthopaedic sandal with two six-degrees-of-freedom force/moment sensors beneath the heel and the forefoot. Moreover, an inertial sensor is rigidly attached to each force/moment sensor. Fusion of CoP with double integrated GRF data is based on a frequency domain method. A detailed description of the method can be found in [2].

## RESULTS

The figure on the right shows a top view of the CoM trajectory of a stroke patient estimated by the ambulatory (solid) and reference system (dashed). Moreover, the CoP on either side of the CoM is indicated by the dots. The root-mean-square difference between the CoM magnitudes estimated by both measurement systems averaged over 100 trials was  $0.025 \pm 0.007$  m (mean  $\pm$  standard deviation).

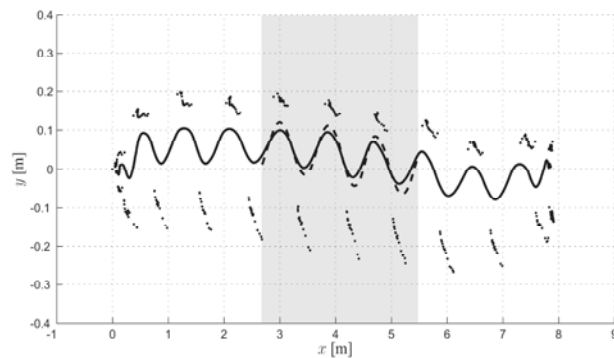

## CONCLUSION

This study has shown the possibility to estimate CoM movement using an ambulatory measurement system. The accuracy was verified by a comparison with an optical reference system. The results are comparable to those described in literature [1].

## ACKNOWLEDGEMENT

This study was financially supported by the Dutch Ministry of Economic Affairs under the FreeMotion project and ZonMW (grant number: 1435.0026).

## REFERENCES

- [1] Eames, M.H.A. et al. Comparing methods of estimating the total body centre of mass in three-dimensions in normal and pathological gaits. *Human Movement Science*, 18(5), 637-646, 1999.
- [2] Schepers, H.M. et al. Ambulatory estimation of center of mass displacement during walking. Submitted.